



# Dario™ User Guide



Thriving with diabetes, together.



© 2014 LabStyle Innovation™ Ltd., ALL RIGHTS RESERVED

## BASIC INFORMATION

Please read this user guide thoroughly and feel free to contact our customer support ([www.mydario.com](http://www.mydario.com)) or your healthcare provider with any questions, concerns or remarks you may have.

LabStyle Innovation™ Ltd.  
9 Halamish St.  
North Industrial Park  
Caesarea 3890000  
Israel

[www.mydario.com](http://www.mydario.com)

Dario™ is a trademark of LabStyle Innovation™ Ltd.

European Patent application number 11780305.6

CE  
0344

6031-01 Rev03

  
DARIO



# TABLE OF CONTENTS

## CHAPTER 1 - INTRODUCTION & USER SAFETY

Glucose Monitoring for a Mobile Age .....	1
Intended Use .....	1
Contraindications .....	2
About These Instructions for Use .....	2
Before Testing With Dario™ .....	2
Safety Definitions .....	2
Cautions .....	3
Notes .....	3
Practices Used in This Advanced User Guide .....	3
Procedure Instructions .....	3
Symbols and Descriptions .....	4
Additional Information .....	5

## CHAPTER 2 - DARIO™ SYSTEM OVERVIEW AND FEATURES

Your Dario™ System at a Glance .....	6
Dario™ Components .....	6
Getting Started With Dario™ .....	9
Assembling the Dario™ System for the First Time .....	9
Inserting the Test Strip Cartridge .....	10
Inserting a Lancet .....	11
Setting Lancet Depth (Optional) .....	12
The Dario™ Application .....	12
Downloading & Installing the Dario™ Application .....	13
Creating Your Account & Personalizing Your Settings .....	14
Setting Your Personal Profile .....	16

## CHAPTER 3 - CHECKING YOUR DARIO™ GLUCOSE METER

Control Test Principle .....	18
Chemical Composition .....	19
Control Solution .....	19
Checking Your Glucose Meter With Dario™ Control Solutions .....	20
Removing the Glucose Meter From the Housing .....	20
Removing a Test Strip From the Cartridge .....	21
Performing a Control Test .....	22
Checking the Glucose Meter With the Check Strip .....	25

## CHAPTER 4 - TESTING YOUR BLOOD GLUCOSE LEVEL

Blood Glucose Testing Precautions .....	27
Test Strip Precautions .....	28
Factors That Interfere With Blood Glucose Testing .....	29
Interpreting the Results .....	29
Measurement Range .....	30

Factors That May Lead to Inaccurate Results .....	30
Step One - Inserting a New Lancet Into the Lancing Device.....	31
Step Two - Removing the Glucose Meter From the Housing.....	33
Step Three- Remove a Test Strip From the Cartridge.....	34
Step Four - Testing Your Blood Glucose.....	35
Performing a Glucose Test .....	36
Step Five - Returning the Meter to the Dario™ Housing.....	40
Test Limitations.....	40
Performance Analysis .....	41

## **CHAPTER 5 - CLEANING AND MAINTENANCE**

Cleaning.....	42
---------------	----

## **CHAPTER 6 - TROUBLESHOOTING**

Troubleshooting.....	43
Problem Solving.....	46

## **CHAPTER 7 - TECHNICAL INFORMATION & SPECIFICATIONS**

How the Glucose Meter Works.....	48
Compatibility.....	48
Technical Specifications .....	48
Compliance With International Standards.....	49
Disposing of Your Meter.....	50

## **CHAPTER 8 - WARRANTY, REPAIRS SERVICE & SUPPLIES**

Repair Policy .....	51
Manufacturers One Year Warranty .....	51
Service Support.....	52
Supplies and Accessories.....	52

# CHAPTER 1 - INTRODUCTION & USER SAFETY

## GLUCOSE MONITORING FOR A MOBILE AGE

Congratulations on your choice of the Dario™ Blood Glucose Monitoring System (BGMS). Dario™ was created to make life easier for people with diabetes - with the right tools, information and support in your pocket. It is a smartphone-based monitoring system, featuring a pocket-sized meter with an integrated lancing device and test strips, combined with an easy-to-use mobile application.

Living with diabetes is a daily challenge. But with Dario™ in your pocket and the best support, we can thrive with diabetes together.

This user guide will guide you through the proper setup and use of your new Dario™ BGMS. We suggest that you read this guide thoroughly in order to familiarize yourself with the system and its many features

## INTENDED USE

The Dario™ BGMS is intended for determination of blood glucose values using fresh capillary whole blood from the fingertip.

The Dario™ BGMS is indicated for the quantitative measurement of glucose in fresh capillary whole blood samples drawn from the fingertips.

The system is intended to be used by a single patient and should not be shared.

The Dario™ BGMS is intended for self-testing outside the body (in vitro diagnostic use) by people with diabetes at home as an aid in monitoring the effectiveness of diabetes control.

The Dario™ BGMS is not to be used for the diagnosis of or screening of diabetes or for neonatal use.

The Dario™ Blood Glucose Meter (BGM) **must** be used with Dario™ blood glucose test strip, Dario™ control solutions, Dario™ lancets and Dario™ application software.

## CONTRAINDICATIONS

The Dario™ BGMS should **not** be used:

- To diagnose diabetes.
- On children younger than four weeks old.
- To test blood taken from an artery or vein.

Glucose monitoring with the Dario™ BGMS is not recommended for independent use by people who are:

- Unable to follow the instructions provided with the system.
- Visually impaired.

## ABOUT THESE INSTRUCTIONS FOR USE

### Before Testing With Dario™

Please read this User Guide carefully and thoroughly before testing your blood glucose for the first time. These instructions will provide you with all the information you need for safe use and handling of your Dario™.

Incorrect use of this system, or failure to apply, implement or follow the instructions and important information contained in this User Guide, may lead to a misdiagnosis or damage to your device.

If you have any questions, please contact customer support at [www.mydario.com](http://www.mydario.com).

### Safety Definitions

Safety instructions are provided for the protection of Dario™ system users. This User Guide includes three types of important messages: Warnings, Cautions and Notes. Text marked with one of these symbols requires your attention to ensure safe and accurate use of your Dario™ system.

### Warnings



**Warning:** indicates precautions needed to prevent **possible risk of injury or damage to your health.**

Do not proceed beyond a Warning message until you fully understand the conditions and you have taken the appropriate preventive action.

## Cautions



Caution

**Caution:** indicates precautions needed to prevent **damage to your monitoring system**.

Do not proceed beyond a Caution message until you fully understand and observe the indicated conditions.

## Notes



Note

Notes are used to provide additional information for the purpose of clarification.

## Practices Used in This Advanced User Guide

### Procedure Instructions

- When appropriate, procedures start with a “❖” symbol, followed by a short description of the procedure to be performed.
- Procedure instructions are clearly identified and presented as numbered procedure steps.
- If relevant, a system response is written below the procedure step and appears in italics.
- All procedures should be done in the order of the steps provided.



Note

The examples and screen images used in this user guide are provided as examples only (unless stated otherwise).

Words in:	Description
<b>Bold</b>	Names of menus, buttons and screens
<i>Italics</i>	System response that occurs as a result of a button press
<b><i>Bold Italics</i></b>	Used to emphasize important information

## SYMBOLS AND DESCRIPTIONS

The following table shows a list of symbols which may appear throughout this guide, on packaging or package inserts, or on the actual system parts. An explanation is provided next to each symbol.

Symbol	Description	Symbol	Description
	Dario™ logo		LabStyle Innovation™ logo
	Consult instructions for use		Do not use if seal is broken or missing
	In Vitro Diagnostic		Batch code
	Expiry date		Shelf life following first opening
	Do not reuse		Temperature limitation
	Catalogue number		Contents
	Manufacturer: LabStyle Innovation™ Ltd. 9 Halamish St. North Industrial Park Caesarea 3890000 Israel		Authorized Representative in the European Community; MDSS GmbH Schiffgraben 41 30175 Hannover, Germany
	Intended for self-testing		Sterilized using Gamma Radiation
	Keep away from sunlight		Keep Dry

Symbol	Description	Manufacturer
	Dario™ Blood Glucose monitoring system Under Directive IVDD 98/79/EC	LabStyle Innovation™ Ltd.
	Dario™ Lancing Device Under Directive MDD 93/42/EEC	LabStyle Innovation™ Ltd.
	Sterile Lancets (25) Under Directive MDD 93/42/EEC	Gentrol Co., Ltd.

## GENERAL PRECAUTIONS

This section informs you of potential hazards which may harm your Dario™ system or cause it to not function properly:

Avoid using any system parts with broken seals or expired “use by” dates. Do not attach or use a component if it is damaged in any way, as it may not work properly.

- The Dario™ system is not water-resistant and should not get wet. If it does get wet, wipe it with a clean dry cloth.
- Blood glucose testing with Dario™ should only be done in temperatures between 10°C - 45°C (50°F - 113°F). Test results may not be correct if the room temperature is outside this range.
- Changes or modifications to the Dario™ system not expressly approved by LabStyle Innovation™ Ltd. will void your warranty and could cause you harm.
- Avoid testing with your Dario™ system in altitudes higher than 3,400 meters (11,155 feet), as accuracy cannot be assured.
- Do not leave the meter in very hot or cold places. Do not leave it near a heat source (radiator) or in a car in hot or cold weather.
- Do not store or use meter or test strips in high humidity, such as a bathroom or kitchen.

## ADDITIONAL INFORMATION

For your safety, please observe the following recommendations when monitoring your blood glucose using the Dario™ system:

- It is always a good idea to have a back-up testing method available. Failure to test could cause a delay in treatment decisions and lead to a serious medical condition. Examples of back-up testing methods include a back-up glucose meter device or testing by a laboratory. Ask your healthcare provider about other possible back-up methods.
- It is recommended that you periodically compare the test results from your Dario™ BGMS with another test system that you know is well-maintained and monitored by a healthcare provider.
- Do not change your treatment based on a single result that does not match how you feel or if you believe that your test result could be incorrect.
- Never make significant changes to your diabetes control program or ignore physical symptoms without consulting with your healthcare professional.

## CHAPTER 2 - DARIO™ SYSTEM OVERVIEW AND FEATURES

This section provides an overview of the Dario™ system components and how it is set up for the first time.

### YOUR DARIO™ SYSTEM AT A GLANCE



The Dario™ is a compact “all-in-one” glucose monitoring system that incorporates a lancing device, a disposable strip cartridge and a miniature glucose meter that snap into a durable pocket-sized housing. The miniature glucose meter attaches to your smart mobile device (see [Compatibility on page 48](#) for a list of devices), which supports you daily with personalized tracking, knowledge about your glucose trends and actionable insights.


- The system is discreet and compact. The entire system easily fits in your pocket.
- By connecting to your smart mobile device, it eliminates the need for additional hardware.
- No coding is required. Insert a Dario™ test strip and you are ready to test.
- Testing is easy. No navigating or buttons to press.
- Actionable insights and alerts – allows easy analysis of trends and behavior.
- Instant sharing with caregivers – allows sharing your data with your caregivers for efficient diabetes management.

### Dario™ Components

Your Dario™ system components are described in the table below.

Component	Description	Image
Housing	The modular Dario™ housing has a built-in lancing device, slots and covers for the snap-in components (lancet, test strip cartridge, and glucose meter).	

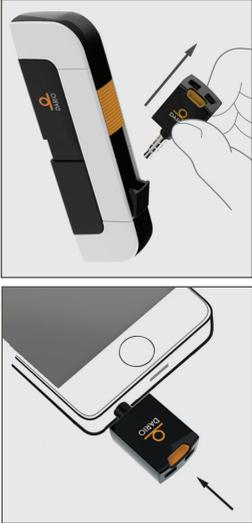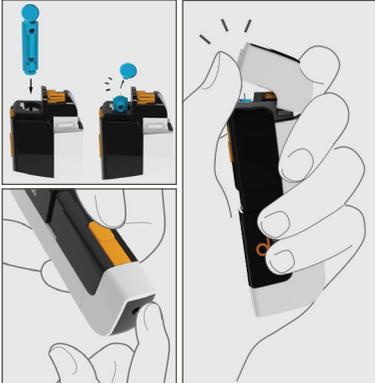Component	Description	Image
<p>Glucose meter</p>	<p>The miniature glucose meter has:</p> <ul style="list-style-type: none"> <li>• An audio connector that is plugged into the headphone socket of the smart mobile device</li> <li>• A strip port for insertion of the test strip.</li> </ul> <p>The glucose meter receives its power from the mobile device and does not require batteries or any other electrical source. When not in use, the meter snaps into its slot in the housing for protected storage.</p>	
<p>Lancing Device and Cover</p>	<p>The lancing device is built into the housing and uses disposable Dario™ lancets. The lancing device cover prevents the user from unintentional punctures. Lancets are changed for each use. Puncture depth may be adjusted, by removing the cover and moving the depth selection dial. The cover is then put back on for use. The lancing device is activated by sliding it with two fingers until it clicks and then pressing the release button. Instructions on using the lancing device are included in <a href="#">Performing a Glucose Test on page 36</a>.</p>	
<p>Test Strip Cartridge</p>	<p>Each test strip cartridge holds 25 strips. The cartridge snaps into the modular Dario™ housing.</p>	

Component	Description	Image
Test Strip	The Dario™ test strip is the only strip which may be used with the Dario™ system. A new test strip is inserted into the test strip port of the glucose meter prior to each glucose measurement.	
Lancets	Dario™ uses a 30G lancet. The lancet is replaced by removing the lancing device cover, pulling out the used lancet and replacing it with a sterile one.	



Note

It is recommended that you carry spare cartridges and lancets in case of an emergency.

## DARIO™ SYSTEM WELCOME KIT CONTENTS



Note

Once you remove the exterior packaging, you will find a white package with a tamper-proof seal. If the tamper-proof seal is missing, it is recommended that you return this Dario™ System to where you purchased it, as it has been opened.

As soon as you receive your Dario™ System Welcome Kit:

- Carefully unpack the kit and verify that it contains the following parts:
  - Dario™ System including Blood Glucose Meter
  - Accessories:
    - ◆ Test strip cartridge (25 strips)
    - ◆ Sterile Lancets (25 lancets)
    - ◆ Check Strip (1 strip)
  - Documentation: User Instructions Short Guide and a Quick User Guide.
- If anything is missing, please contact customer support at [www.mydario.com](http://www.mydario.com).

## GETTING STARTED WITH DARIO™

Your Dario™ meter works seamlessly with your smart mobile device. Simply download the Dario™ application on your smart mobile device and it will automatically synchronize with the Dario™ device each time it is connected.

Your data is constantly synchronized to one place so that it is always with you on the go, so you can stay in control of your health.

Your data is saved under your username on your smart mobile devices and on the Dario™ cloud, with easy access through the Dario™ application and also My Dario™ website.

So let's get started!

## ASSEMBLING THE DARIO™ SYSTEM FOR THE FIRST TIME

Setting up the Dario™ System for the first time includes the following steps described in this section:

- Inserting a test strip cartridge (see [Inserting the Test Strip Cartridge on page 10](#))
- Inserting a lancet (see [Inserting a Lancet on page 11](#))
- Setting lancet depth (optional) (see [Setting Lancet Depth \(Optional\) on page 12](#))
- Downloading the Dario™ application to your smart mobile device (see [Downloading & Installing the Dario™ Application on page 13](#))
- Setting up the Dario™ application on your smart mobile device using the Dario™ app instructions or the instructions provided on the Dario™ website.



Note

Both ends of the housing have covers that are removable. The lancet cover is the one with the small opening. Please be careful not to put the cartridge cover on the lancing end. This can damage the lancet and the lancing device.


## Inserting the Test Strip Cartridge

### ❖ To insert the test strip cartridge:

Remove the cartridge cover of the Dario™ housing by pushing it outwards (from the side with the removal indication lines) until it comes off.



1. Remove the new test strip cartridge from its pouch.
2. Hold the test strip cartridge with the side that opens, on top (as shown below).

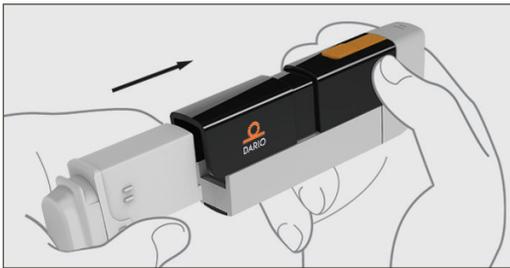

3. Insert the cartridge into the housing until it snaps into place.
4. Replace the housing cover by sliding it into place until it clicks.





If the cover does not close properly, the cartridge may not have been inserted correctly.


## Inserting a Lancet

### ❖ To insert a lancet:

1. Remove the Lancet Device Cover (the end with the small opening) from the Dario™ housing.



2. Remove a new lancet from the packaging.
3. Insert a sterile lancet as far as it will go and make sure it is firmly set.

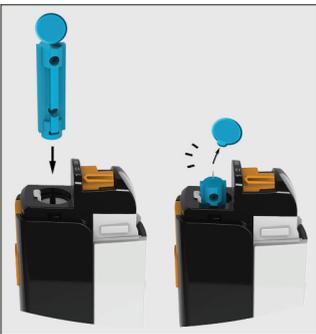


4. Carefully twist off the lancet cap. Make sure not to bend the lancet while removing the cap.

## Setting Lancet Depth (Optional)


The depth of the lancet, as it punctures the skin of your fingertip, can be adjusted by moving the lever between the numbers one to four (printed on the dial). One (1) is the shallowest depth and (4) is the deepest. It is recommended to start with your lancet depth set to level one and adjust the level if necessary.

### ❖ To set lancet depth:

1. Move the lancing device lever so that the line on the lever is aligned with the correct depth.

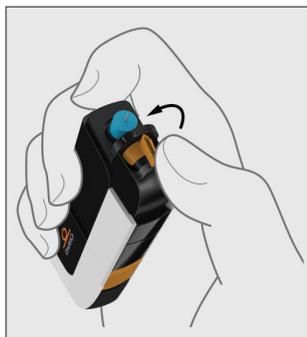

2. Return the lancing device cover by sliding it into place until it clicks. Be careful not to touch or bend the lancet.

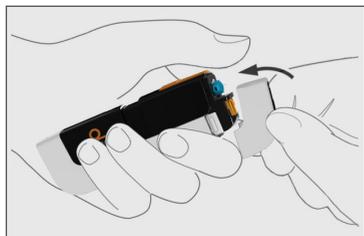

## THE DARIO™ APPLICATION

Your Dario™ meter is operated via the app displayed on the screen of your smart mobile device. The mobile device receives information from the glucose meter, displays and stores it. The app also provides a step-by-step Quick Guide for operating the system. Additionally, you can find more instructions on the Dario™ Application User Guide at [www.mydario.com](http://www.mydario.com).

Instructions for downloading the app are provided in the next section.

The app can be used to conveniently store and manage your diabetes information, review trends or share information with your healthcare provider.

## Downloading & Installing the Dario™ Application

You can download and install the Dario™ app to your smart mobile device using the Apple App Store. The app is downloaded and installed the same way as other Apps on your smart mobile device. The Dario™ app is free of charge and is customized for your smart mobile device.



Note

Downloading the app from the App Store requires data connectivity.



Note

For accurate use of the Dario™ system with the app, the time and date must be correctly set on your smart mobile device. For instructions on setting the time and date on your device, please refer to the support materials for the device.

### ❖ To download the Dario™ App:

1. Turn on your smart mobile device and launch the **App Store** app. Alternately, for quicker access, you can use an app that scans codes to scan the following code.



2. Search for the **Dario™** app by LabStyle Innovation™ Ltd (Health & Fitness category) and tap on the Dario™ icon.
3. Tap **Free** and then tap **Install**.
4. Enter your App Store password information as required.

*The application downloads. Once installed, the orange Dario™ icon appears on your smart mobile device home screen.*



Note

The Dario™ app needs to be installed once for each of your smart mobile devices.



Note

Updates may be downloaded periodically from the App Store.

## Creating Your Account & Personalizing Your Settings

### ❖ To setup your Dario™ App:

1. After installing the Dario™ app on your mobile device, click on the orange Dario™ icon . The icon appears on your mobile device Home screen.

*The Dario™ LOG IN/SIGN UP screen appears.*



2. Select **SIGN UP** to register as a Dario™ user.
3. In the **SIGN UP** screen, input your First Name, Last Name, E-mail and a Password. You must also Confirm your Password and agree to the **Terms and Conditions** by tapping on the circle so that a check mark appears.
4. Continue by following the instructions on the screen to sign up.



Note

Your password must have at least seven characters, an upper case letter, a lower case letter and a number.




Note

Your e-mail address and password will be used for future login to the app and to the Dario™ web-portal.



Note

If you already have a Dario™ account, you may skip this section.

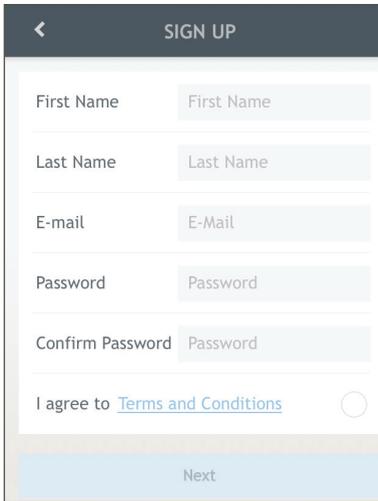

The screenshot shows a 'SIGN UP' form with the following fields and elements:


- First Name: Input field with placeholder text 'First Name'
- Last Name: Input field with placeholder text 'Last Name'
- E-mail: Input field with placeholder text 'E-Mail'
- Password: Input field with placeholder text 'Password'
- Confirm Password: Input field with placeholder text 'Password'
- I agree to [Terms and Conditions](#): A checkbox next to the text.
- Next: A blue button at the bottom of the form.

5. Press **Next** when done.



If nothing happens when you press **Next**, verify that you agreed to the Terms and Conditions.

*You are automatically brought to the Personal Profile Screen.*

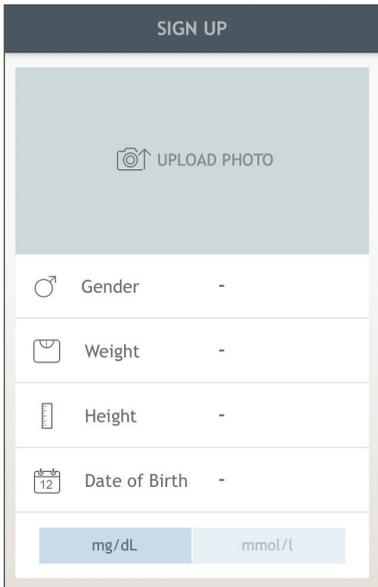

The screenshot shows the 'SIGN UP' screen with the following elements:

- UPLOAD PHOTO: A button with a camera icon and an upward arrow.
- Gender: A dropdown menu with a male symbol icon and a '-' sign.
- Weight: A dropdown menu with a scale icon and a '-' sign.
- Height: A dropdown menu with a ruler icon and a '-' sign.
- Date of Birth: A dropdown menu with a calendar icon and a '-' sign.
- mg/dL: A button with a blue background.
- mmol/l: A button with a light blue background.



Note

You can edit your e-mail address and password and set the Dario™ app language and region by going to the menu and then selecting **SETTINGS > ACCOUNT SETTINGS**.

## Setting Your Personal Profile

### ❖ To set your personal profile:



Note

If you do not want to setup your profile at this time, you can tap **SKIP** and continue to setting your Diabetes Profile.


1. **Optional:** Enter your Gender, Weight, Height and Date of Birth. It is also possible to upload a photo from your device by tapping **UPLOAD PHOTO**.
2. Select your preferred measurement unit system (mg/dL or mmol/L) by tapping either the **mg/dL** button or **mmol/L** button.
3. Press **DONE**.



Note

You can update your settings at any time by tapping the Menu icon  in the top left corner and selecting **SETTINGS**.

*A screen appears with the option to do a Walkthrough (help) or to get started.*

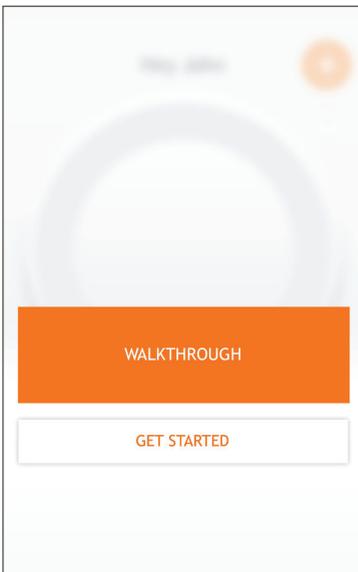


5. Select **GET STARTED**.



Note

You can do the Walkthrough at any time by tapping the  icon. Select **HELP > APP WALKTHROUGH**.

*The First Entry screen appears.*

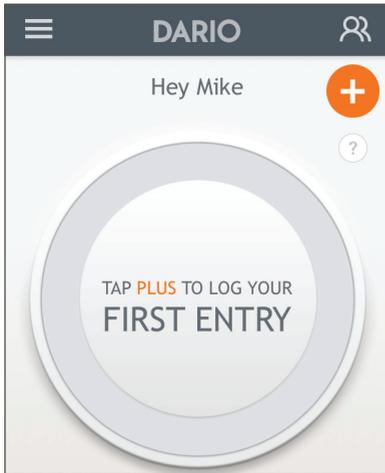

6. We advise you to continue setting your Diabetes Profile, following the app instructions. Completing your profile will allow full app functionality.

## CHAPTER 3 - CHECKING YOUR DARIO™ GLUCOSE METER

This section provides information on checking the accuracy of your meter.

There are two ways of testing the accuracy of your glucose meter.

- **Control Solution** - Confirms that the meter and test strips are performing as expected. A drop of control solution is placed on a test strip (using a piece of paper). Compare the results on the meter with the values displayed on the test strip cartridge.
- **Check Strip** - Confirms that the meter is performing as expected. The reusable check strip that is supplied with the Welcome Kit is used to test the meter's performance.

To ensure that your results are always accurate, you need to check the performance of your meter in the following cases:

- If you drop the meter.
- Whenever your result does not match the way you feel.
- If you have repeated a test, and the blood glucose result is still lower or higher than expected.
- When you open a new test strip cartridge.
- Whenever you want to check the performance of a meter and test strip.

### CONTROL TEST PRINCIPLE

Dario™ Glucose Control Solution contains a known amount of glucose that reacts with chemicals on the Dario™ test strip.

When applying a drop of control solution to the test strip, following the same procedure that is used for whole blood, the glucose in the control solution reacts with chemicals in the test strip.

The result displayed on the meter should fall within the expected range printed on the test strip container label. Obtaining a single result within the expected range is sufficient to verify system performance. A result outside the range printed on the Test Strip container label may indicate the system is not performing correctly.



Note

This control solution is not for use as a cleaning solution.

## CHEMICAL COMPOSITION

Dario™ Glucose Control Solution is an aqueous solution, which contains D-glucose as the reactive ingredient in the approximate concentration.

- Buffer 75mM
- Polyvinylpyrrolidone 5%
- Polyvinyl alcohol 5%
- SDS 0.1%
- Preservative 0.1%

## CONTROL SOLUTION

Dario™ Control Solution package can be ordered separately. Please contact your local representative for ordering information. Dario™ Control Solution package comes with two bottles of control solution (H and M types).

- Avoid contact with the eye. Contact your healthcare professional immediately if solution is swallowed, injected, or applied to the eye.
- Dye in control solution may stain skin, clothing, or surfaces.
- Store the control solution between 8°C-30°C (46°F-86°F). Keep away from direct sunlight, fluorescent light, and heat. Do not freeze.
- Once you open a new bottle of control solution, mark the opening date on the bottle.
- Make sure that your control solution has not expired. Check the expiration date on the bottle.
- Make sure that your control solution was not opened more than 3 months ago.
- Keep the control solution away from children.
- Shake the control solution well before using.
- Wipe the container tip clean after use and be sure to close the container tightly after each use.
- No reconstitution or dilution of the control solution is necessary.

## CHECKING YOUR GLUCOSE METER WITH DARIO™ CONTROL SOLUTIONS

The following steps are required to perform a control solution test.

### Removing the Glucose Meter From the Housing

Before performing a control solution test, it is necessary to remove the glucose meter from the housing.

The glucose meter is stored in the housing when not in use.




Caution

When not in use, store the meter in the Dario™ housing. Do not leave your meter connected to your smart mobile device with the screen in ON mode for more than two (2) minutes, as it can get warm and can affect accuracy.

#### ❖ To remove the meter from the housing:

1. Hold the housing so that the ridged orange panel is close to you and the end with the lancing device is facing away from you.
2. Slide your thumb back on the ridged orange panel.

*The meter will pop up.*

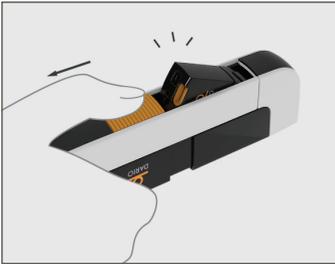

3. Grasp the meter with two fingers and remove from the housing.





Caution

**Do not** plug the Dario™ meter into any device other than a compatible smart mobile device audio socket. The list of compatible smart mobile devices is provided in [Chapter 7 – Technical Information & Specifications](#)

## Removing a Test Strip From the Cartridge

You should have a test strip cartridge already inserted in your Dario™ housing. If this is not the case, please go to [Inserting the Test Strip Cartridge on page 10](#).

### ❖ To remove a test strip from the cartridge:

1. Remove the Cartridge Cover of the Dario™ housing by pushing it outwards until it comes off (use the removal indication lines).



2. Snap open the case by pushing up the edge.



3. Remove a test strip from the cartridge.



4. Snap the case closed immediately and replace the cartridge cover by pushing it into place until it clicks.



Note

It is recommended to use the test strip immediately after removing it from the cartridge. It is recommended **not** to use a test strip that has been outside of the cartridge for more than three (3) minutes.



Note

If the cover does not close properly, the cartridge may not have been inserted correctly.




Caution

- Do not touch the yellow testing site when handling the test strip.
- Do not use a damaged test strip.

## Performing a Control Test

### ❖ To perform a control test.

1. Tap the Dario™ icon on your smart mobile device to launch the Dario™ application.

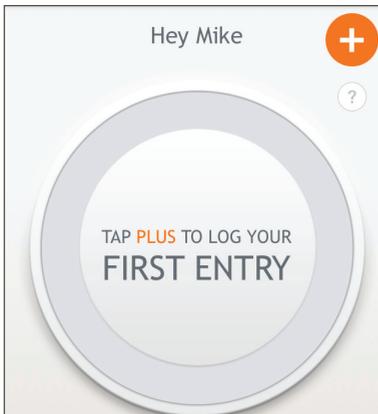

2. Insert your meter into the audio plug of your smart mobile device.




A *Connecting...* message appears, followed by *INSERT A NEW STRIP.*




Note

Verify that the meter is inserted as far as it can go into the socket of the smart mobile device.

3. Hold the test strip with the gold contacts facing the meter.
4. Without bending the strip, insert it into the test strip port (marked in orange) of the Dario™ glucose meter as far as it will go.

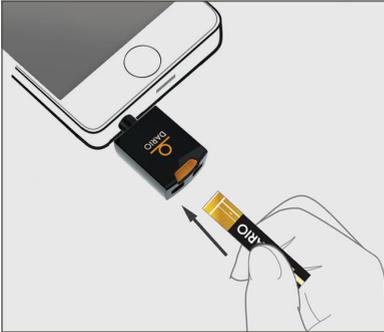


You are instructed to place a drop of blood on the test strip.

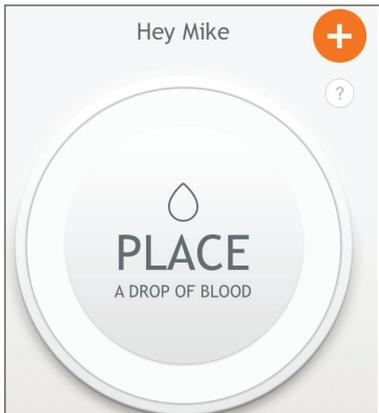

5. Shake the control solution container and apply a drop of control solution to a piece of paper.
6. Hold the paper and move it so that the solution touches the tip of the yellow window of the strip.
7. **Important:** Verify that enough control solution is applied to fill the window so that it turns red. Do **not** put control solution on top of the test strip.

When the meter detects that the solution was applied, the “Measuring...” message appears. The orange rotating in the circle indicates that the test is in progress.

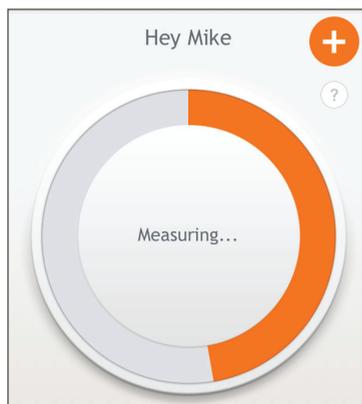

8. The test result appears on the screen after six (6) seconds. Read your result and look at the test strip .

*The glucose test result is automatically saved to memory. The result appears on the screen and is automatically saved to memory.*



Note

It is possible to delete this control test from memory, if desired.

For more information, refer to the Dario™ Application User Guide at

[www.mydario.com](http://www.mydario.com).

9. When the test is done, remove the test strip.
10. Compare the results on the meter with the values displayed on the test strip cartridge.
11. If the results are:
- within the acceptable range, then your meter is ready for use.
  - outside of the acceptable range, perform the test again. If the problem recurs, contact customer support at [www.mydario.com](http://www.mydario.com).
12. Disconnect the meter from your smart mobile device.
13. Wipe the tip of the control solution container clean and tightly seal the container.



Note

The Dario™ Glucose Control Solution ranges printed on the test strip cartridge label are intended for the Dario™ test strip cartridge only.



Note

The glucose concentrations in these solutions, when measured by systems other than Dario™ Glucose Monitoring System, may differ.



Note

Applying too much or too little control solution to the test strip may cause out- of-range results.



Caution

Do not use your Dario™ Glucose Monitoring System to test your blood if your control solution result falls outside of the acceptable range.


**14.** Place the meter back into the housing:

- a. Hold the meter at a angle with the part that connects to the smart mobile device facing away from the ridged orange panel.
- b. Push the meter into the housing at an angle and then push downwards until the meter clicks into place.



## CHECKING THE GLUCOSE METER WITH THE CHECK STRIP

1. Open the Dario™ application.
2. Connect the Dario™ meter to the smart mobile device as described in the previous section.
3. Insert the Dario™ Check Strip into the test strip port. A **Check strip detected** message appears. *The border of the circle is gradually filled with blue, indicating that the test is in progress.*

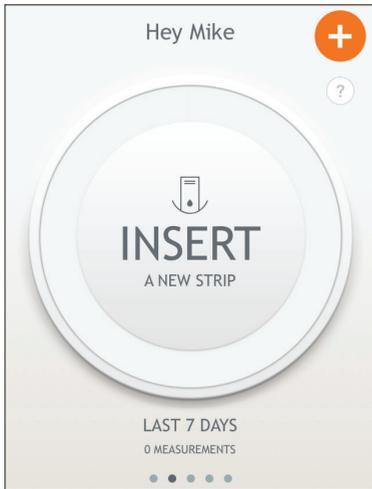

4. Within six (6) seconds, the test is completed and one of two messages appears:

Message	Recommended Action
<b>Check strip verified successfully</b>	Proceed with blood glucose testing.
<b>Error- check strip measurement is out of range (0)</b>	<ul style="list-style-type: none"> <li>• Do not use the Dario™ meter.</li> <li>• Contact customer support at <a href="http://www.mydario.com">www.mydario.com</a>.</li> </ul>

## CHAPTER 4 - TESTING YOUR BLOOD GLUCOSE LEVEL

This section provides information on testing your blood glucose with your meter.

Before using your Dario™ for the first time, we recommend to verify that the system gives accurate results. Check the performance of your glucose meter by following the [Checking Your Glucose Meter With Dario™ Control Solutions on page 20](#) and [Checking the Glucose Meter With the Check Strip on page 25](#).

Do not use the system if control solution result is out of range.

The glucose meter in Dario™ measures the amount of glucose in your blood. Once placing a small drop of blood from your fingertip onto the test strip, the result will be displayed in six (6) seconds.

Carefully read and follow the instructions provided in this chapter and in the package inserts for the test strips and control solutions. It is very important to follow the instructions in order to prevent an incorrect result or improper treatment.



Caution

Do not put any fluid into the test strip port.

Once you start your Dario™ app, follow the prompts on the screen.

### BLOOD GLUCOSE TESTING PRECAUTIONS



Warning

The meter, test strips, and control solutions are only for use outside the body (in vitro). Do not eat the test strips. Do not swallow or inject control solutions, or use control solutions for any purpose other than testing your blood glucose.

Incorrect test results can cause the wrong therapy recommendation to be made and may lead to serious adverse health effects. Therefore, please follow these instructions carefully.

## Test Strip Precautions

- Only use Dario™ test strips. Using other test strips with this glucose meter can produce inaccurate results.
- Inspect each test strip cartridge before opening it for the first time. If you see any damage to the cartridge lid, or if anything prevents the lid from closing properly, do not use the test strips.
- Run a control test every time you open a new test strip cartridge. For additional information, see [Checking Your Glucose Meter With Dario™ Control Solutions on page 20](#).
- Store unused test strips in their original cartridge. Do not remove test strips from the test strip cartridge and put them into another container.
- Close the cartridge tightly right after you remove a test strip. This helps keep the test strips dry.
- Be sure to check the “Use by” date on the test strip cartridge. Do not use the test strips after that date.
- Be sure to write down the date the strips were first opened. Check the date when using the strips. If the date surpasses the shelf life after first opening, do not use the strips from this cartridge.
- Use the test strip immediately after removing it from the cartridge.
- Use the test strips as indicated in this guide.
- Do not store your test strips in temperatures below 2°C (36°F) or above 32°C (90°F).
- Do not refrigerate your test strips. Do not put them in a freezer.
- Do not expose your test strips to direct sunlight, moisture or humidity, which can damage your test strips and lead to inaccurate results.
- Do not apply blood or control solution to the test strip before inserting it into the glucose meter.
- Do not reuse test strips. Once control solution or blood is placed on a test strip, discard the strip. If you need to retest, use a new test strip.
- Do not bend, cut, or alter the test strips.
- Do not get dirt, food, or other material on the test strip.
- It is recommended to use the test strip immediately after removing it from the cartridge. It is recommended **not** to use a test strip that has been outside of the cartridge for more than three (3) minutes.
- Do not touch the yellow testing site when handling the test strip.

- Do not use a damaged test strip.
- Make sure that the gold contact area of the test strip is clean from dirt, blood, moisture and anything else. These items will affect the test result and can cause an inaccurate blood glucose level result.

## FACTORS THAT INTERFERE WITH BLOOD GLUCOSE TESTING

- Certain substances can interfere with the blood glucose system and cause falsely high results. For more information, refer to the test strip package insert. If you are taking medication or dietary supplements, consult your doctor.



Caution

You should not use this system to test your blood glucose if you are critically ill (examples include: severe hypotension or shock, hyperglycemic-hyperosmolar state, hypoxia, diabetic ketoacidosis). Certain health conditions, such as serious illness and dehydration, can cause falsely high test results in glucose meters. If you are very sick or think you are dehydrated, or are urinating frequently, call your doctor immediately.



Note

Dirty or wet hands could affect your results. Alcohol can affect test results.

## INTERPRETING THE RESULTS

If the displayed test result reflects the way you feel, continue as instructed by your doctor.



Warning

If the test result does not reflect the way you feel, please check your Dario™ system by running a control solution check ([Performing a Control Test on page 22](#)). Repeat the blood glucose test afterward. If your blood glucose result still doesn't match how you feel and you have followed the instructions provided here, follow your healthcare provider's instructions.



Warning

Do not change your treatment based on a single result that does not match how you feel or if you believe that your test result could be incorrect. The blood glucose reading displayed on your smart mobile device by Dario™ BGMS should not be the only information you use to make decisions about your health. Always consult a health care professional to interpret and understand the measurement results.

## MEASUREMENT RANGE

Your meter measures blood glucose results in the range of 10 mg/dL to 600 mg/dL (0.6-33.3 mmol/L). Results that are outside of this range should be reviewed according to the procedure below.

- If your test result is lower than 10 mg/dL (0.6 mmol/L), "**LOW!**" is displayed instead of a result.



Warning

LOW may indicate that your blood glucose is very low (possibly severe hypoglycemia). Follow your doctor's instructions immediately and repeat the test.

- If the result is higher than 600 mg/dL (33.3 mmol/L), "**HIGH!**" is displayed instead of a result.
- If your blood glucose test results in a LOW or HIGH message, repeat the blood glucose test following all of the instructions provided in [Step Four - Testing Your Blood Glucose on page 35](#).
- If your blood glucose test results in a LOW or HIGH message a second time, follow the protocol established by your health care professional or contact your healthcare provider immediately.
- Please note that the exact blood glucose reading that constitutes a HIGH or LOW reading depends on many factors, including individual differences, and the time since your last meal.

## FACTORS THAT MAY LEAD TO INACCURATE RESULTS

Certain medications, food supplements, medical treatments and health conditions can interfere with the blood glucose system and cause inaccurate results.

Incorrect testing technique or improper storage or handling of the Dario™ may also lead to implausible test results which don't match the way you feel. These include:

- Your hands may not have been washed thoroughly
- Your glucose meter test strip port may be contaminated.
- Your test strip has been bent.
- The test strip is expired. Check the "use by" date.
- The length of time that has passed since first opening the test strip package exceeds the allowed time.

- Test strips were stored incorrectly.
- Testing was done in a humid environment (for humidity specifications, refer to [Technical Specifications on page 48](#)).
- Your glucose meter has been dropped.



Note

If your meter has been dropped and you are receiving error messages or implausible results, contact customer support.



Warning

Do not rely on the blood glucose measurement alone in making health care decisions.

## STEP ONE - INSERTING A NEW LANCET INTO THE LANCING DEVICE



Note

Use a new sterile lancet in your lancing device every time you test your blood glucose to prevent infection.


### ❖ To insert a lancet:

1. Remove the Lancet Device Cover from the Dario™ Housing.



Note

You can identify the Lancet Device Cover by the small opening in the cover.

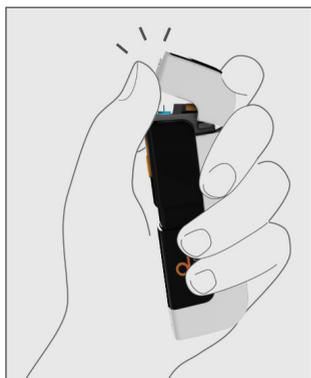


**2. Remove the used lancet as follows:**

- a. Pull the tab next to the lancet holder with your thumb.
- b. Press the orange button firmly with your other hand to keep lancet position and pull the lancet out of the lancing device.

If you prefer, it is possible to remove the lancet by grasping it and pulling it straight out of its housing.



Dispose of used lancet in a safe manner so as not to cause accidental injury.

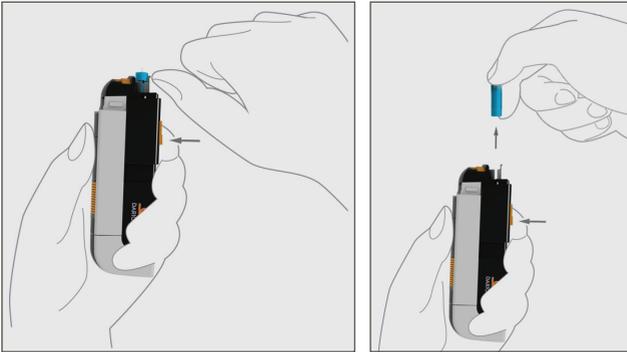


**3. Remove a new lancet from the packaging.**



Do not use the lancet if the cap is missing or damaged. Please contact customer support at [www.mydario.com](http://www.mydario.com).

**4. Insert a sterile lancet and make sure that it is firmly in place.**

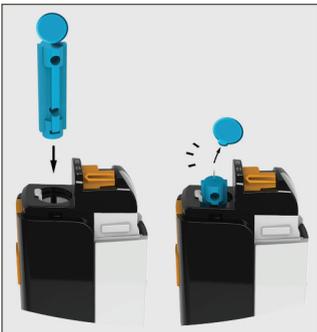



Caution

- Only use a lancet authorized by LabStyle Innovation™ (30G).
  - If the lancet does not click into place or the lancet holder does not hold the lancet properly, insert another sterile lancet.
  - If the problem persists, it may be necessary to replace your Dario™ housing. Contact Customer Support at [www.mydario.com](http://www.mydario.com).
5. Carefully twist off the lancet cap as shown above. Make sure not to bend the lancet needle.
  6. If necessary, set the depth of the lancing device. For additional information, see [Setting Lancet Depth \(Optional\)](#) on page 12.
  7. Replace the lancing device cover by sliding it into place until it clicks. Be careful not to touch or bend the lancet.

## STEP TWO - REMOVING THE GLUCOSE METER FROM THE HOUSING


Before starting the testing procedure, you should remove the meter from the housing.

The meter is stored in the housing when not in use.

### ❖ To remove the meter from the housing:

1. Hold the housing so that the ridged orange panel is close to you and the end with the lancing device is facing away from you.
2. Slide your thumb back on the ridged orange panel.

*The meter will pop up.*

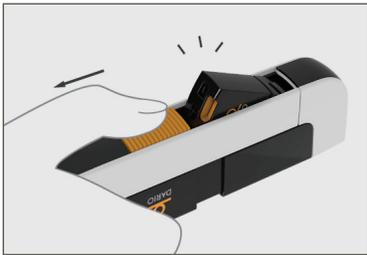

3. Grasp the meter with two fingers and remove from the housing.



Caution

**Do not** plug the Dario™ meter into any device other than a compatible smart mobile device audio socket. The list of compatible smart mobile devices is provided in [Chapter 7 - Technical Information & Specifications](#).

## STEP THREE- REMOVE A TEST STRIP FROM THE CARTRIDGE

You should have a test strip cartridge already inserted in your Dario™ housing. If this is not the case, please go to [Inserting the Test Strip Cartridge on page 10](#).

1. Wash your hands with warm soapy water and dry thoroughly. If you use alcohol wipes to cleanse fingers, make sure the area is completely dry before lancing finger.
2. Remove the Cartridge Cover of the Dario™ housing by pushing it outwards until it comes off (use the removal indication lines).



3. Snap open the case by pushing up the edge.



4. Remove a test strip from the cartridge.



5. Snap the case closed and replace the housing cover by sliding it into place until it clicks.



Note

If the cover does not close properly, the cartridge may not have been inserted correctly.

## STEP FOUR - TESTING YOUR BLOOD GLUCOSE

### Testing Information and Guidelines

- The meter requires only a small drop of blood, about the size of a sugar grain (0.3 $\mu$ L), to perform the test. For best results, select a puncture site along the side of a fingertip.
- Testing blood from sites other than the fingertip may give inaccurate results.

- If too little blood is applied to the test strip, an alert informs you that your sample size is too small and you should try again with a new strip.
- If a test strip error occurs, perform another test with a new test strip.
- Blood glucose results are automatically saved to memory. The results remain on the screen for 15 minutes.
- If an error message or symbol appears on the screen, refer to [Chapter 6 - TROUBLESHOOTING](#) for additional information.
- Dirty or wet hands could affect your results. Alcohol can affect test results.
- ***When not in use, store the meter in the Dario™ housing. Do not leave your meter connected to your smart mobile device with the screen in ON mode for more than two (2) minutes, as it can get warm and can affect accuracy.***




Caution

To prevent malfunction of the meter, keep the test strip port free of blood, moisture, dirt, or dust. Always store the glucose meter in the Dario™ housing when not in use.

## Performing a Glucose Test

1. Tap the Dario™ icon on your smart mobile device to launch the Dario™ application.

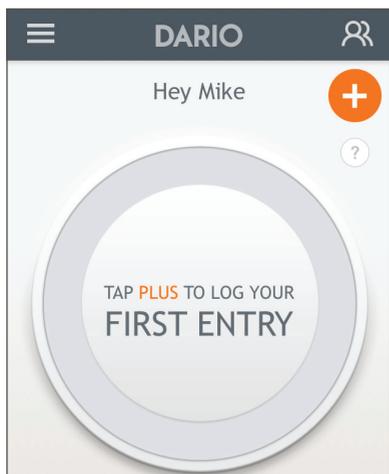

2. Insert your meter into the audio plug of your smart mobile device. Verify that the meter is inserted as far as it can go into the socket of the smart mobile device.




*A Connecting... message appears, followed by INSERT A NEW STRIP.*

3. Hold the test strip with the gold contacts facing upward.
4. Without bending the strip, insert it into the test strip port of the Dario™ glucose meter as far as it will go.




*You are instructed to place a drop of blood on the test strip.*

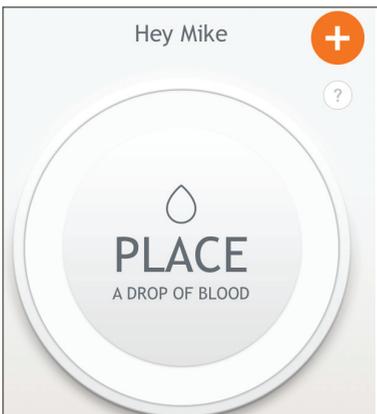

5. Set the lancing device for activation by sliding it with two fingers until it clicks.



6. Place the lancing device cover (side with the small opening) to the side of your fingertip and press the release button to prick your finger.




7. Apply a drop of blood to the tip of the yellow window of the test strip. Capillary action will pull the blood into the strip.



8. **Important:** Verify that enough blood is applied to fill the window so that it turns red. Do **not** put blood on top of the test strip.

When the meter detects that blood has been applied the “Measuring...” message appears. The border of the circle is gradually filled with orange, indicating that the test is in progress.

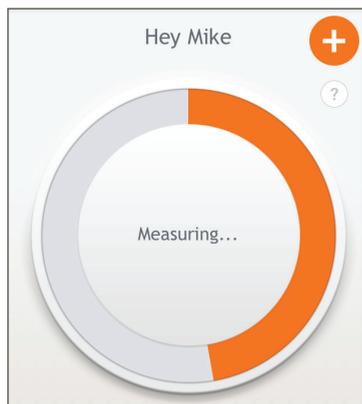

- Remove your finger from the strip once the message appears.



Warning

Do not add blood to the test strip once you have removed your finger, as you may receive an inaccurate result.

- The test result appears on the screen after approximately six (6) seconds. Read your result.

*The glucose test result is automatically saved to memory. If for some reason you do not see a result, go to your Logbook (see Dario™ app User Guide on the Dario™ website).*



Warning

If a phone call is received during a measurement, the test will be stopped and will not be saved. A message **test strip is used** will appear on the result screen.

- When the test is done, remove the test strip. Dispose of the test strip as per local regulations for bio-hazardous waste.
- Remove the lancet from the lancing device (see [page 32](#)). Dispose of the used lancet according to local guidelines.

*When the test strip is removed from the glucose meter, the message “Please insert new test strip” appears.*

- You may continue to input data into your Dario™ application. For more information, refer to the Dario™ Application User Guide at [www.mydario.com](http://www.mydario.com).

14. Return the meter to the housing as described in the next section.

## STEP FIVE - RETURNING THE METER TO THE DARIO™ HOUSING

### ❖ To return the meter to the Dario™ Housing:

1. Disconnect the meter from your smart mobile device.
2. Hold the meter at a angle with the part that connects to the smart mobile device facing away from the ridged orange panel.
3. Push the meter into the housing at an angle and then push downwards until the meter clicks into place.

## TEST LIMITATIONS

Normal endogenous (within body) natural levels of uric acid, ascorbate (vitamin C), bilirubin, triglycerides, and hemoglobin do not interfere with your blood glucose results. Elevated levels of these compounds in your blood may, however, interfere with the accuracy of your blood glucose results obtained with the Dario™ System. The system should not be used if blood levels of these compounds exceed the limitations detailed in the table below.

Compound	Limitation
Ascorbic acid	> 4 mg/dL
Uric acid	> 9 mg/ dL
Acetaminophen	> 6 mg/dL
Total bilirubin	> 40 mg/dL
Triglycerides	> 1,026 mg/ dL

The drugs L-dopa, dopamine, methyl-dopa, acetaminophen, and ibuprofen will not interfere with Dario™ system blood glucose results when taken at therapeutic concentrations.

Patients undergoing oxygen therapy may yield false results.

## PERFORMANCE ANALYSIS

The performance data for the Dario™ system was obtained using capillary blood from diabetic patients (method comparison, accuracy), venous blood (repeatability) and control solution (reproducibility). The system is calibrated with venous blood containing various glucose concentrations. The reference values for this were obtained using the hexokinase method. For method comparison, the results were compared with results obtained using the hexokinase method with deproteination (automatic analyser). The hexokinase method is traceable to a NIST standard.

## CHAPTER 5 - CLEANING AND MAINTENANCE

This section provides cleaning and disinfecting information for your meter.

The Dario™ Glucose Monitoring System should be cleaned once a week and disinfected once a month.

### CLEANING

If your Dario™ components are soiled, the outer surfaces may be wiped with a soft, lint-free cloth slightly dampened with mild soap and water solution or 70% ethyl alcohol.

Clean the Dario™ Blood Glucose Monitoring System with IPA 70% (isopropanol) wipes (Medline, USA) once a week and with the disinfection agent Super Sani Cloths Wipes once a month.

#### **Do not:**

- Expose the device to solvents
- Get any moisture in the test strip slot
- Spray any cleaning solution directly onto the glucose meter or the lancing device
- Submerge any part of the Dario™ in liquid
- Attempt to clean any internal parts
- Attempt to dry any parts using a blow dryer

Please observe the following cautions when cleaning the Dario™ system to avoid damaging the device:



Caution

If the device becomes wet, wipe off all moisture and allow sufficient time for drying before using.



Caution

Contact with solvents can cause severe deterioration of plastic parts and malfunctioning of the instrument and accessories.

### DISINFECTING


Disinfection should be performed with PDI Super Sani Cloth Germicidal Wipes.

## CHAPTER 6 - TROUBLESHOOTING

In this chapter you will find information about all the symbols and error messages which may be displayed on the Dario™ app. To ensure safe and accurate use of Dario™, please pay attention to all symbols and messages when you use the system. They provide you with important information.

If you still have questions after reading this chapter, contact customer support at [www.mydario.com](http://www.mydario.com).

An error message can appear as a popup or as a message within the main circle.

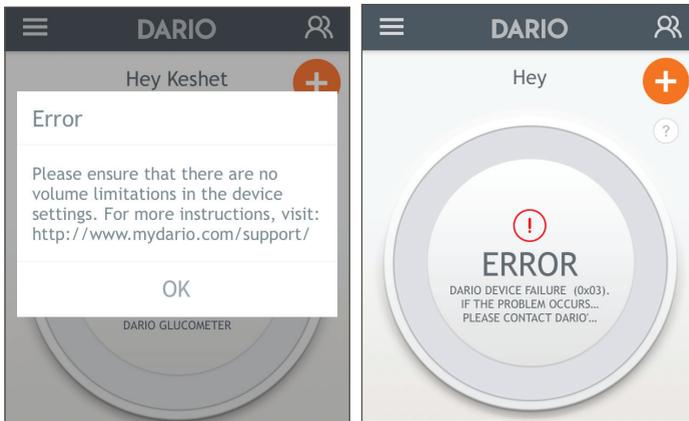

### TROUBLESHOOTING

The following table lists some typical conditions that may occur with the Dario™ System.

Message Content	Possible Cause / Recommended Action
<p>Please ensure that there are no volume limitations in the device settings. For more instructions, visit:  <a href="http://www.mydario.com/support/">http://www.mydario.com/support/</a></p>	<p>Smart device volume setting inappropriately.</p> <p>Check the following settings in your mobile device:</p> <ol style="list-style-type: none"> <li>1. Make sure that <b>Mono Audio</b> is set to off: <ul style="list-style-type: none"> <li>• Verify that <b>Mono Audio</b> is set to off.</li> </ul> </li> <li>2. Adjust the audio balance: <ul style="list-style-type: none"> <li>• <b>Settings &gt; General &gt; Accessibility &gt; Hearing</b></li> <li>• The audio volume balance must be set in the middle between L and R.</li> </ul> </li> <li>3. Make sure that your Ringer and Alerts volume is set to the maximum: <ul style="list-style-type: none"> <li>• <b>Settings &gt; Sounds</b></li> <li>• Look at the <b>RINGER AND ALERTS</b> section and make sure that it is set to the maximum volume (all the way to the right).</li> </ul> </li> <li>4. Allow Dario™ to use your microphone: <ul style="list-style-type: none"> <li>• <b>Settings &gt; Privacy &gt; Microphone</b></li> <li>• Make sure that the Dario™ app is set to on (green).</li> </ul> </li> <li>5. Make sure that your music volume is set to the maximum: <ul style="list-style-type: none"> <li>• <b>Settings &gt; Music &gt; Volume Limit</b></li> <li>• Make sure that it is set to the maximum volume (all the way to the right).</li> </ul> </li> </ol>
<p>Insufficient blood detected, try again with a new strip</p>	<p>Not enough blood on the strip.  Repeat the measurement with a new strip.</p>
<p>The Strip is used, please insert a new strip</p>	<p>A strip was used more than once.  Perform a new measurement with a new strip</p>

Message Content	Possible Cause / Recommended Action
High! Measure with a new strip, if recurs contact your physician Immediately	<p>High glucose level.</p> <p>Measurement result is above 600 mg/dL (33.3 mmol/L). Repeat the measurement with a new strip. If this recurs, contact your physician Immediately. If your measurement results are inconsistent with the way you feel, contact customer support at <a href="http://www.mydario.com">www.mydario.com</a>.</p>
Temperature out of range. Move to an area between 10-45°C (50°-113°F), wait 30 minutes and try again	<p>The meter was left in an extreme temperature environment.</p> <p>Move to a cooler or warmer area, wait at least 30 minutes and repeat the measurement with a new strip.</p>
Dario™ device failure (0x01). If the problem occurs again, please contact Dario™'s customer support	<p>Firmware software failure.</p> <p>Contact customer support at <a href="http://www.mydario.com">www.mydario.com</a>.</p>
Dario™ device failure (0x02). If the problem occurs again, please contact Dario™'s customer support	<p>Voltage Failure</p> <p>Contact customer support at <a href="http://www.mydario.com">www.mydario.com</a>.</p>
Unknown device, please connect Dario™	<p>Another device is inserted into the smart mobile device's audio connector.</p> <ul style="list-style-type: none"> <li>• If another device is connected to the earphone plug, disconnect it in order to connect Dario™. You can still use the Dario™ app if another device is connected.</li> <li>• If you received this message while the Dario™ meter is connected, disconnect and reconnect the meter. If this message still appears, contact customer support at <a href="http://www.mydario.com">www.mydario.com</a>.</li> </ul>
Hypo warning	<p>Hypoglycemia event occurred</p> <p>You received a measurement result lower than defined in the hypo warning section under <b>Blood Glucose Thresholds</b> (see <a href="#">page 46</a>) in your Diabetes Profile. Contact your physician immediately.</p>
Check strip measurement is out of range. If this problem occurs again, please contact Dario™'s customer support	<p>Fault in check strip or meter.</p> <p>Repeat the check strip measurement again. If the error recurs, contact customer support at <a href="http://www.mydario.com">www.mydario.com</a>.</p>

## PROBLEM SOLVING

### Test strip inserted but “Please insert a new strip” keeps appearing on the screen.

The test strip was removed before the reading was completed or strip or meter are defective.

- Repeat the measurement, using a new test strip.
- Check the meter with a check strip (see [Checking the Glucose Meter With the Check Strip on page 25](#)). If the result is not okay, contact customer support at [www.mydario.com](http://www.mydario.com). If the result is okay, test with a new test strip.

### Cannot pierce skin with lancet.

- The needle depth may be incorrect. Adjust the lancet depth lever to a different depth level.
- The lancet needle may be bent. Replace the lancet.
- The cartridge cover may be in the place of the lancing device cover. Please be careful to return each cover to the correct end.

### The lancet does not fit correctly into the lancing device.

The lancet may be faulty or you may be using a lancet that is not approved for use with the Dario™ System. Replace the lancet with a different Dario™ lancet. If the problem persists, you may need to replace the Dario™ housing. Contact customer support at [www.mydario.com](http://www.mydario.com).

### Cannot remove the used needle from the lancing device.

The lancet may be faulty or you may be using a lancet that is not approved for use with the Dario™ System. Pull the needle carefully and straight out from lancet.

### Lancing Device does not operate correctly.

The lancing device spring or handle may be faulty. Make sure that you set the lancing device for activation by sliding it with two fingers until it clicks (see [page 38](#)). Then you can press the button to puncture your skin.

### Lancet Depth Indicator lever is stuck.

The indicator lever may be faulty. Replace the Dario™ housing. Contact customer support at [www.mydario.com](http://www.mydario.com).

### Lancing Device release button does not work properly.

The lancing device is faulty. Replace the Dario™ housing. Contact customer support at [www.mydario.com](http://www.mydario.com).

### “Strip is used and should be replaced” message appears.

An incoming phone call during blood testing will result in this message appearing. It is recommended to set your smart mobile device to flight mode before performing a test.

### Forgotten Dario™ password.

If you forget your password, tap on **FORGOT PASSWORD** in the **LOG IN** screen. An email with instructions for resetting your password will be sent to you.

### My smart mobile device battery died.

If the battery of your smart mobile device is out of power, use a different device. Download the Dario™ application and login to your account.

## CHAPTER 7 – TECHNICAL INFORMATION & SPECIFICATIONS

This section provides technical information on your Dario™ System.

### HOW THE GLUCOSE METER WORKS

The Dario™ system determines the amount of glucose in fresh capillary blood using electrochemical biosensor technology. An electrical current is generated by the reaction of glucose with the reagent on the test strip (glucose oxidase). The strength of the current produced by the reaction depends on the amount of glucose in the blood sample. The glucose meter detects the current and converts it into a blood glucose reading.

### COMPATIBILITY

Dario™ is compatible for use on smart mobile devices. For full list of compatible devices please refer to [www.mydario.com/support/getting-started/](http://www.mydario.com/support/getting-started/)

### TECHNICAL SPECIFICATIONS

Meter Specifications	
Result Range	10-600 mg/dL (0.6-33.3 mmol/L)
Calibration	Plasma-equivalent
Sample	Fresh capillary whole blood
Test Sample	0.3 microliter
Test Time	6 seconds
Assay Method	Glucose Oxidase Biosensor
Hematocrit Range	20% - 60%

Accuracy	<ul style="list-style-type: none"> <li>for glucose concentrations &lt; 4,2 mmol/L (75 mg/dL), the percentage of results within + 0,28 mmol/L, + 0,56 mmol/L and + 0,83 mmol/L (+ 5 mg/dL, + 10 mg/dL and + 15 mg/dL) of the reference values</li> <li>for glucose concentrations &gt; 4,2 mmol/L (75 mg/dL), the percentage of results within + 5 %, + 10 %, + 15 % and + 20 % of the reference values</li> </ul>
Power Supply	Powerless
Glucose Units	mg/dL, mmol/L
Dimensions	104x211x11 mm (4.1x8.3x.4 in)
Weight	40 gram (1.4 oz)
Memory	Unlimited results Memory is limited to smart mobile device memory
Average	7-day, 14-day or 30-day averaging
Display	Dario™ application on a smart mobile device screen
Function	Hypo warning: Set by user.
<b>Glucose Meter/Lancing Device</b>	
Operational Temperature	10°C-45°C (50°F-113°F)
Storage Temperature Strip	2°C-32°C (36°F-90°F)
Altitude	Up to 3,400 meters (11,155feet)
<b>Test Strip</b>	
Operational Temperature	10°C-45°C (50°F-113°F)
Storage Temperature Strip	2°C-32°C (36°F-90°F)
Operational Altitude	Up to 3,400 meters (11,155feet)



Note

Do not store near solvents and ionizing radiation source.

## COMPLIANCE WITH INTERNATIONAL STANDARDS

This meter meets the electromagnetic immunity requirements as per EN ISO 15197 Annex A. The chosen basis for electrostatic discharge immunity testing was basic standard IEC 61000-4-2. In addition, it meets the electro-magnetic emissions requirements as per EN 61326. Its electromagnetic emission is thus low. Interference from other electrically driven equipment is not to be anticipated.

## DISPOSING OF YOUR METER

The product may come into contact with blood during measurement. Used products therefore carry a risk of infection.

Please dispose of used products according to the regulations applicable in your country. For information about correct disposal, please contact your local council or authority.

The product falls outside the scope of the European Directive 2002/96/EC (Directive on waste electrical and electronic equipment (WEEE)).

## CHAPTER 8 - WARRANTY, REPAIRS SERVICE & SUPPLIES

This section provides repair, warranty, service support and ordering information for your Dario™ System.

### REPAIR POLICY

When under warranty, repair and service must be performed by LabStyle Innovation™ Ltd. When the LabStyle Innovation™ warranty is not applicable, repairs may be performed by LabStyle Innovation™ Ltd. or authorized representatives, on a parts and labor basis.

After replacement, verify that the unit is fully functional by performing the normal setup procedure.



Do not remove the covers of the device components. Only perform maintenance procedures specifically described in this user guide.

### MANUFACTURERS ONE YEAR WARRANTY

It is important to LabStyle Innovation™ Ltd. that you are completely satisfied with your Dario™ BGMS. LabStyle Innovation™ Ltd. warrants your new Dario™ will be free from defects in materials and workmanship for a period of one (1) year from the date of the original purchase. If during this time the Dario™ does not work properly because of a defect in materials or workmanship, LabStyle Innovation™ Ltd. agrees to replace or repair, free of charge any and all parts proven to be defective and subject to warranty. This warranty is in lieu of all other warranties, expressed or implied, including any implied warranty of merchantability or fitness for any purpose, other than stated herein. This warranty does not apply to the performance of a Dario™ BGMS that has been damaged by accident or has been altered, misused, tampered with, or abused in any way. This warranty only applies to the original purchaser of the meter and/or its agents.

## SERVICE SUPPORT

Repairs of the Dario™ System under warranty must be made at authorized repair centers. If the device needs repair, contact LabStyle Innovation™ Ltd. service department or your local distributor.

If you need to ship the device, please pack the device and its accessories carefully to prevent shipping damage.

## SUPPLIES AND ACCESSORIES

Dario™ BGMS supplies and accessories are available from LabStyle Innovation™ Ltd. or from your local distributor. For a list of distributors, please visit [www.mydario.com](http://www.mydario.com).

Item	Catalog Number
System	1015-01
	Dario™ Welcome Kit
Test Strip Cartridge	1016-01
	Dario™ Test Strip (1 x 25)
	1024-01
	Dario™ Test Strip (2 x 25)
Lancet	1018-01 Dario™ Lancet (1 x 100)
	1019-01 Dario™ Lancet (1 x 25)
Control Solution	1054-02 Dario™ Control Solutions (2X1.25ml) H
Check Strip	1034-01 Dario™ Check Strip
Software	1022-01
	Smart mobile device software application ver 2.x

Life is easier  
with Dario™ in your pocket

